



Instruction for use
Tango shower toilet chair



Instruction for use

Tango

5100 5700

shower toilet chair

Basic UDI-DI: 872025610305951005700LK



If caregivers have a choice

Important:

Read these instructions carefully before using the Tango!

Date first used.....

User.....

Name.....

Address.....

Manufacturer

Lopital Nederland B.V.

Laarakkerweg 9

















5061 JR Oosterwijk

T +31 (0)13 5239300

www.lopital.nl

info@lopital.nl

All of the aids produced by Lopital comply with the applicable standards for Class I medical products (MDR (EU) 2017/745).

Explanation of symbols in 'instruction for use' and on labels			
	Note		Follow the instructions for use.
	Date of production		Read cleaning and disinfecting protocol.
	Manufacturer information		Antibacterial
	Article number		Temperature
	Serial number		Air pressure
	Conformité Européenne		Humidity level
	Medical device		Maximum load
	GS1 Datamatrix containing the following information: (01) Global Trade Item Number (internationally unique item number) (11) Production date (21) Serial number		Keep the device away from heat, hot surfaces, sparks, open flames, and other ignition sources. No smoking.

Contents

1.	Introduction	5
1.1.	Introduction	5
1.2.	Safety.....	5
1.3.	Warranty.....	7
2.	Use	7
2.1.	First use.....	7
2.2.	Working with the Tango.....	9
3.	Operation.....	10
3.1.	Wheel blocking.....	10
3.2.	Footrests.....	10
3.3.	Armrests.....	10
3.4.	Toilet function.....	11
3.4.1.	In combination with toilet	11
3.4.2.	Use of a bedpan or bucket	11
4.	Cleaning and maintenance.....	12
5.	Environmental conditions	14
6.	Removal of parts.....	14
7.	Technical specifications.....	14
7.1.	Structure.....	14
7.2.	Dimensions	14

1. Introduction

1.1. Introduction

The shower toilet chair Tango is a medical device for caring for and washing clients in an ergonomically responsible manner. Comfort is the primary consideration for both the client and the carer. The Tango can also be used as a toilet chair, in combination with a bedpan / bucket. The Tango is a shower toilet chair with independent, folding armrests, polyurethane seat, rails for a bedpan and rotating and foldable footrests.



The frame of the Tango has an antibacterial coating. The coating contains silver ions. Antibacterial coating based on silver ions prevents dangerous micro-organisms such as bacteria, fungi and algae from multiplying and spreading. The effectiveness was confirmed in several tests. Germs were demonstrably reduced in a short time to 99.99%. The coating only affects bacteria that are found on the surface and not on airborne micro-organisms. The coating does not protect users or others from disease-causing bacteria, germs, viruses or other harmful organisms. On a dirty surface, the coating loses its antibacterial properties. So proper cleaning and disinfection is still a must.

The expected technical lifetime of the Tango is 10 years, provided that daily and periodic maintenance is carried out according to the specified maintenance schedule (*See chapter 4. Cleaning and maintenance*).

The Tango is a Class I medical device with CE marking. This marking is in accordance with the regulation MDR (EU) 2017/745.

1.2. Safety



A failure to comply with the following safety points and the further definitions in these instructions for use could lead to hazardous situations. Please read carefully before use.

Use

- Make sure that the Tango brake is applied before transferring clients.
- Notify the client before moving the Tango.
- Make sure that the client always places his/her arms on the armrests provided to prevent possible entrapment.
- Keep the armrests down / closed when moving the Tango.
- Always try to move backwards over obstacles (rather than forwards).
- It is not permitted to charge the Tango with more than 180 kg / 400 lbs.
- The Tango is only suitable for moving and caring for one person.
- Only use original parts, supplied by Lopital.

- Use the Tango in a clean and tidy working environment.
- Swimming pool locations are not considered to be 'normal conditions' and will substantially shorten the lifespan of certain components.
- The Tango cannot be used on a surface with a gradient over 5 degrees laterally.
- The Tango cannot be used on a surface with a gradient of over 10 degrees forwards /backwards.
- The Tango may only be used indoors.

Maintenance

- The Tango must be inspected and serviced at least once a year.
- In the event of damage to the seat, back or backrest, always replace them for reasons of hygiene.
- Servicing and maintenance of the Tango may only be carried out by persons qualified by Lopital.
- Service and maintenance must not be carried out while a client is sitting on the chair.
- If erroneous use, transport, an accident or improper maintenance leads to deformation of the Tango, it may no longer be used and you must contact the supplier.

In the event of breakdowns, you must contact Lopital or your local supplier.

E-mail: info@lopital.nl



The Tango shower toilet chair should only be operated by competent personnel who have experience in working with the user target group and have watched the instruction / training videos on the Lopital website.



The Tango has been developed and produced for use in professional care environments.



Making changes to the construction may affect the safety of the Tango. Furthermore, the liability and guarantee conditions of Lopital lapse. As a result, the Tango no longer complies with the MDR (EU) 2017/745 regulation for medical devices.



If a serious incident occurs related to this medical device that affects the caregiver or the client, it must be reported to Lopital or the distributor of the medical device.

1.3. Warranty

All Lopital products are supplied with a 5-year warranty, on construction and / or material faults, unless otherwise stated. In the event of varying warranty terms, the exact period will be indicated on your invoice; this also serves as the warranty itself. Components and batteries that are subject to wear and tear will not fall under warranty unless there are clear construction and / or material faults.

2. Use

2.1. First use





In the picture below, the components of the Tango are named. In the event of damage, these parts can be replaced by qualified persons.





Scan for
information



 Laarakkerweg 9 5061 JR Oisterwijk The Netherlands T: (+31)13-5239300 CE Weight: -- kg / -- lbs	GTIN (01) 8720256103--	Item no: -----
	 (11) YYMMDD	
	SN (21) ---- -- --	
	 -- kg / -- LBS Product type	



2.2. Working with the Tango

Step 1

If necessary, fold the armrests up (See paragraph 3.3. *Armrests*).

Step 2

If necessary, fold the foot plates up and fold the footrest frame up too (See paragraph 3.2. *Footrests*).

Step 3

The Tango must be put on the brakes before transferring persons (See paragraph 3.1. *Wheel blocking*).

Step 4

The client can take a seat in the chair. Support the client if necessary.

Step 5

Place both feet on the footrests (See paragraph 3.2. *Footrests*).

Step 6

Close the armrests once the client has taken a seat in the chair (See paragraph 3.3. *Armrests*).

Step 7

Notify the client about the processes you will be carrying out.

Step 8

Take the chair off the brakes when you wish to move it (See paragraph 3.1. *Wheel blocking*).

3. Operation

3.1. Wheel blocking

- The brake can be applied on the Tango by pushing the blue lip (1) on the wheel downwards (See figure 1).
- In order to take the Tango off the brake, the same lip on the wheel must be moved upwards by tapping the upper side of the lip (2) (See figure 1).

Option: Directional wheel left front.




Figure 1. Swivel wheel.

3.2. Footrests

- Before the client takes a seat in the Tango, the footrests or footrest frame must be folded upwards. There is now sufficient room to allow the client to easily take a seat (See figures 2 & 3).
- The carer or the client first raises one leg; the carer then folds the footrest (See figure 4). The same procedure is then carried out with the other leg.



Figure 2. Folding up footrests.



Figure 3. Folding up footrest frame.



Figure 4. Folding down footrests.

3.3. Armrests

- The independent folding armrests are easy to fold up.
- Protect the user when moving the armrests upwards / downwards.
- In the folded up position, they should not fall back down by themselves; in other cases: consult your supplier.

Option: Armrests with front closure.

- When the client has taken a seat on the Tango, the armrests with front closure can be folded down; these are then turned in front of the client.
- The armrests with front closure are secured in a horizontal position.
- The armrests can be unlocked by pressing the security catch at the hinging point on the frame (See

figure 6). The armrest can then be turned up for the client and folded up.

- Always protect the client when folding the armrests up or down.
- The armrests can also be used as a support when taking a seat or standing up. Be aware that the armrests are not locked in all positions.

Option: Dual locking.

- The extra lock ensures that the front closure is also locked when turned away (See figure 8).



Figure 5. Armrest Tango.



When folding the armrests away, avoid the hinging point to prevent possible entrapment.



When folding the armrests away, avoid fingers or body parts becoming entrapped between the armrest and the backrest.



The armrests or front closure must not be used as a lever arm (e.g. when moving the chair over an obstacle) or as a push / pull bar. You must not sit on it either. This could damage the Tango and / or present a hazard.



Figure 6. Armrest with front closure.

3.4. Toilet function

3.4.1. In combination with toilet

- The Tango can also be moved over the toilet.
- Remove the inlay from the seat before the person sits down in the chair.
- The Tango can now be moved backwards over the toilet.



Figure 7. Armrest with dual locking.



The Tango does not fit over every toilet.

3.4.2. Use of a bedpan or bucket

- If the Tango is being used as a toilet chair, the special guides under the seat can be used to accommodate a stainless steel / plastic bedpan or bucket.
- The bedpan or bucket is slid in from the back of the chair (See figure 9).
- If you are using the Lopital plastic bedpan, you must slide it as far



Figure 8. Armrest turned out.

forward as possible (See figure 10).

- If you are using a stainless steel bedpan or bucket, the bedpan can be placed in 2 positions under the seat. At the front of the seat (See figure 11) or at the back of the seat (See figure 12).



In order to avoid injuries, we advise the carer to remove the inlay from the seat and insert the bucket or bedpan before the client takes a seat on the chair.



The Lopital plastic bedpan, stainless steel bedpan and bucket must be cleaned and disinfected after use, for example in a bedpan washing unit.



If the Lopital plastic bedpan, stainless steel bedpan or bucket has been used, it must be removed from the chair before the chair is moved or adjusted in height.




Figure 9. Bedpan.



Figure 10. Lopital plastic bedpan.

4. Cleaning and maintenance

The Tango must be cleaned after every use, with water and regular household cleaning agents. PUR integrated foam components with IMC coating should be rubbed clean and disinfected. Do not use any abrasive or other aggressive cleaning products. If necessary, the PUR components can be disinfected with a solution of 70% ethanol or propanol.

The time the products must be left on the components has a significant impact upon the lifespan of the PUR components. As a result of the material properties of PUR, contact with sharp objects must be avoided. This could lead to damage or tears in the material. Finally, we would like to point out that non-critical parts of the PUR components must also be cleaned and disinfected.

Check the wheels regularly for hairs, dust and soap residues and remove when necessary. Maintenance and repairs to the Tango may only be carried out by qualified personnel.



Figure 11. Stainless steel bedpan, front.




Figure 12. Stainless steel bedpan, back.

Maintenance schedule	
After every use	<ul style="list-style-type: none"> • Clean chair with water and regular household cleaning products. • PUR foam components must be cleaned and disinfected. • Check to ensure all parts of the Tango are present, including the footrests, head support and inlay for the seat.
Weekly	<ul style="list-style-type: none"> • Check wheels for hairs, dust and soap residues and remove if necessary. • Check that the chair is still working correctly.
Annually	<ul style="list-style-type: none"> • According to the regulation MDR (EU) 2017/745 medical devices, a chair must be maintained according to the manufacturer's guidelines. This process will preferably be carried out by Lopital or another authorised body. Lopital offers the option of having the chair thoroughly inspected and serviced once a year via Periodic Preventative Maintenance. <p>For more information about the maintenance contract, please contact Lopital (info@lopital.nl) or speak to your supplier.</p>


For a detailed explanation regarding cleaning and disinfecting, see the document 'Cleaning and Disinfection Protocol' on our website www.lopital.com/downloads.

5. Environmental conditions

Conditions during storage and transport

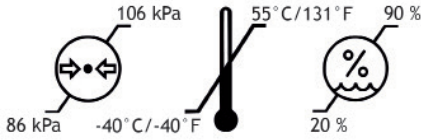

Conditions during use

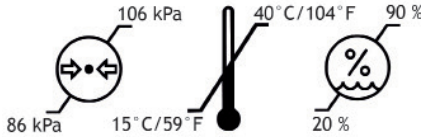

6. Removal of parts

All parts that are replaced or removed can be sent back to Lopital BV. You may also offer the parts to the engineer for destruction. We will ensure that all parts are processed in an environmentally-friendly manner.




7. Technical specifications

7.1. Structure

Frame:	Stainless steel and steel tubes and plates that are equipped with a two-layer powder coating
Hinge points:	Stainless steel
Wheels:	Plastic, Ø 12.5 cm / 4.9 inch, double blocking facility
Body support:	PUR (polyurethane)
Weight:	19 kg / 41.9 lbs
Maximum permitted load:	180 kg / 400 lbs

7.2. Dimensions

Surface area:	66 cm / 26 inch wide, 84 cm / 33.1 inch deep
Seat height:	55 cm / 21.7 inch

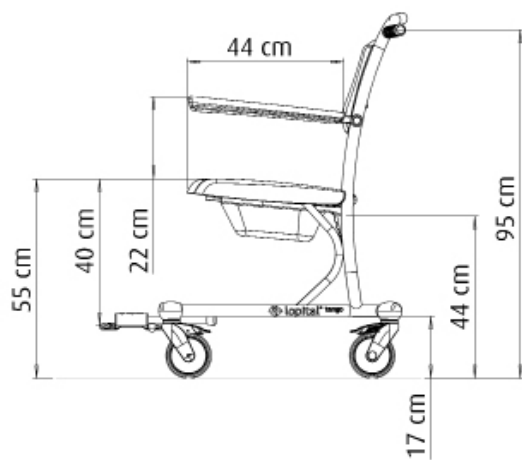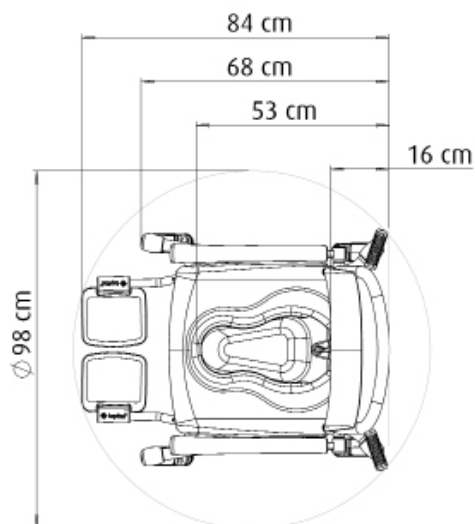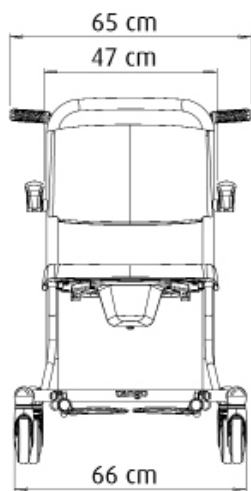



For more information also visit our website: www.lopital.com
Lopital Nederland B.V. Laarakkerweg 9, 5061 JR Oisterwijk, Postbus 56,
5060 AB Oisterwijk, Tel +31 (0)13 52.39.300, E-mail info@lopital.nl,
www.lopital.nl

Copyright ©2026 Lopital. All rights reserved.



Green Deal



ISO CERTIFIED
9001 - 13485 - 14001



Scan for
information